
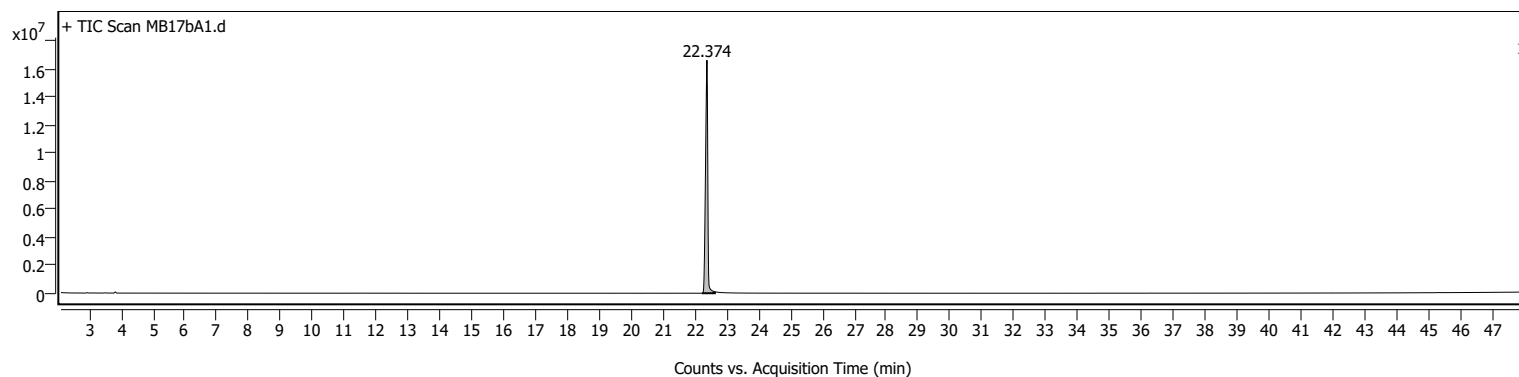


# Analysis Report

## Sample Information

Name	MB17bA1	Data File Path	D:\MassHunter\GCMS\1\data\MB\MB17\MB17bA1.D
Sample ID		Acq. Time (Local)	9/8/2022 4:43:25 PM (UTC+02:00)
Instrument	GCMS	Method Path (Acq)	D:\MassHunter\GCMS\1\methods\Standard HP 5 MS Temp 40 -320C_48min.M
MS Type	Q	Version (Acq SW)	MassHunter GC/MS Acquisition 10.0.384.1 14-Feb-2019 Copyright © 1989-2018 Agilent Technologies, Inc.
Inj. Vol. (ul)	0.5	IRM Status	
Position	134	Method Path (DA)	D:\MassHunter\GCMS\1\data\MB\MB17\MB17bA1.D\Results\Qual\Version4\default.m
Plate Pos.		Target Source Path	
Operator		Result Summary	

## Sample Chromatograms

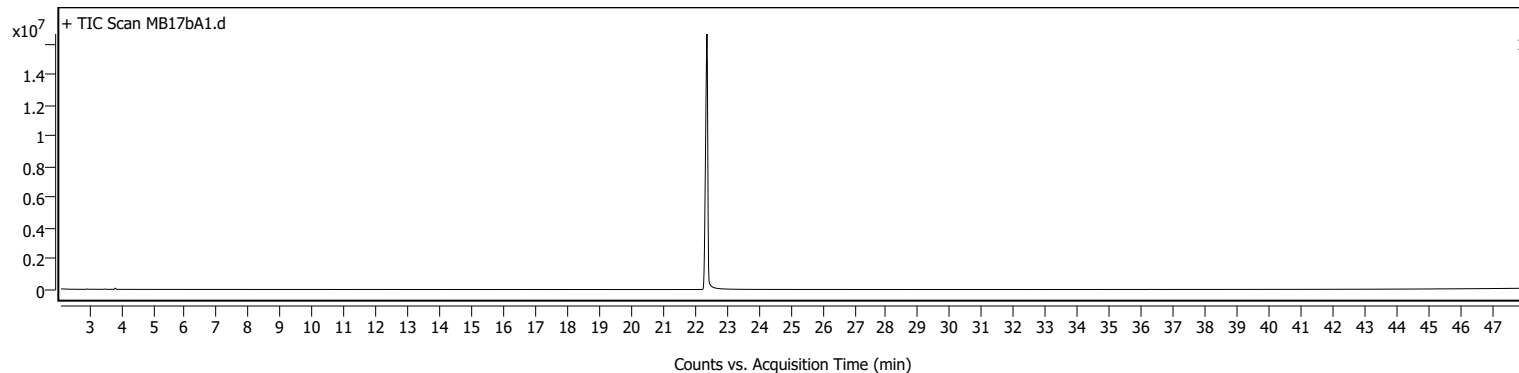


### Chromatogram Peaks

Peak	Start	RT	End	Height	Area	Area %	SNR
1	22.218	22.374	22.622	16611806	82003319	100.00	

## Sample Spectra

### + Scan (rt: 22.36 min)

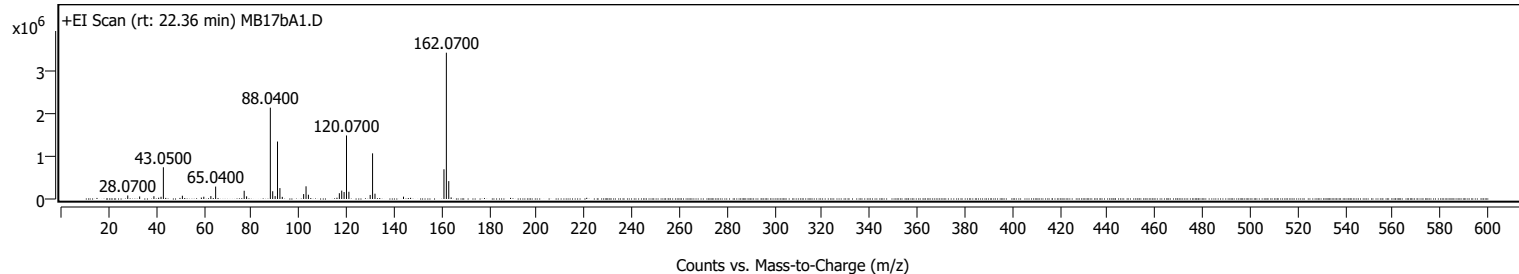

# Analysis Report



Agilent

Trusted Answers

## Spectrum Peaks

m/z	Z	Abund	Abund %	m/z (Calc)	Diff (ppm)	Ion Species	Formula	Ion Type
28.0700		83271	2.41					
33.0800		60073	1.74					
39.0700		66382	1.92					
42.0700		52313	1.51					
43.0500		750276	21.70					
51.0500		77754	2.25					
60.0600		53667	1.55					
63.0300		68865	1.99					
65.0400		293682	8.49					
77.0400		194570	5.63					
78.0500		63102	1.82					
88.0400	1	2158747	62.43					
89.0400	1	183400	5.30					
90.0500	1	68474	1.98					
91.0500		1358348	39.28					
92.0600		257912	7.46					
93.0600		50533	1.46					
102.0400		116289	3.36					
103.0500		299830	8.67					
104.0500		100641	2.91					
117.0600		136648	3.95					
118.0600		198032	5.73					
119.0600		164527	4.76					
120.0700	1	1502126	43.44					
121.0800	1	170845	4.94					
130.0300		95778	2.77					
131.0400	1	1079278	31.21					
132.0400	1	125732	3.64					
144.0400		55041	1.59					
161.0600		702881	20.33					
162.0700	1	3457841	100.00					
163.0700	1	423104	12.24					
164.0700	1	38039	1.10					

MassHunter Qual 10.0  
(End of Report)