
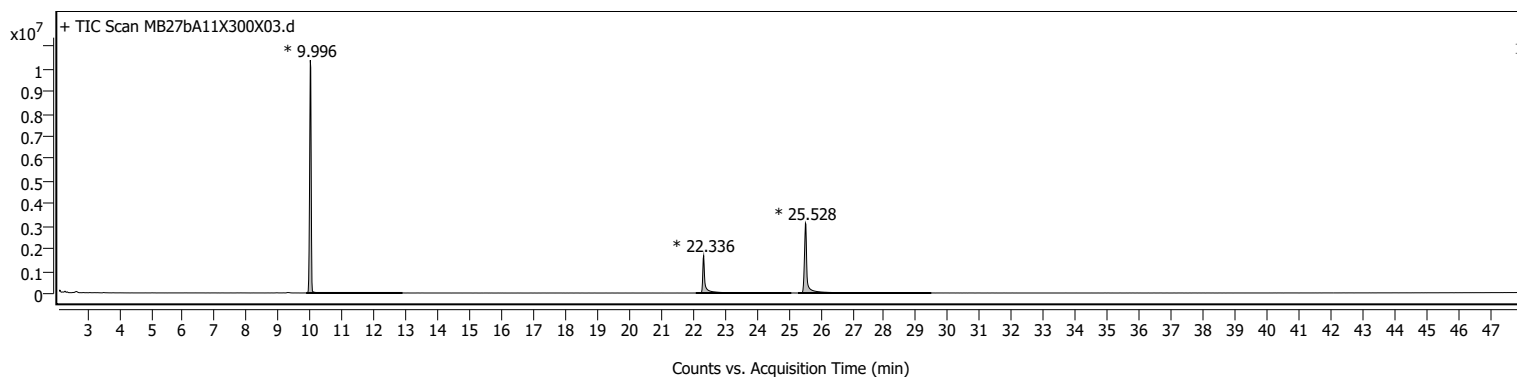


# Analysis Report

## Sample Information

<b>Name</b>	MB27bA11X300X03	<b>Data File Path</b>	D:\MassHunter\GCMS\1\data\MB\MB27\MB27bA11X300X03.D
<b>Sample ID</b>		<b>Acq. Time (Local)</b>	10/14/2022 6:09:42 AM (UTC+02:00)
<b>Instrument</b>	GCMS	<b>Method Path (Acq)</b>	D:\MassHunter\GCMS\1\methods\Standard HP 5 MS Temp 40 -320C_48min.M
<b>MS Type</b>	Q	<b>Version (Acq SW)</b>	MassHunter GC/MS Acquisition 10.0.384.1 14-Feb-2019 Copyright © 1989-2018 Agilent Technologies, Inc.
<b>Inj. Vol. (ul)</b>	0.5	<b>IRM Status</b>	
<b>Position</b>	118	<b>Method Path (DA)</b>	D:\MassHunter\GCMS\1\data\MB\MB27\MB27bA11X300X03.D\Results\Qual\Version4\default.m
<b>Plate Pos.</b>		<b>Target Source Path</b>	
<b>Operator</b>		<b>Result Summary</b>	

## Sample Chromatograms

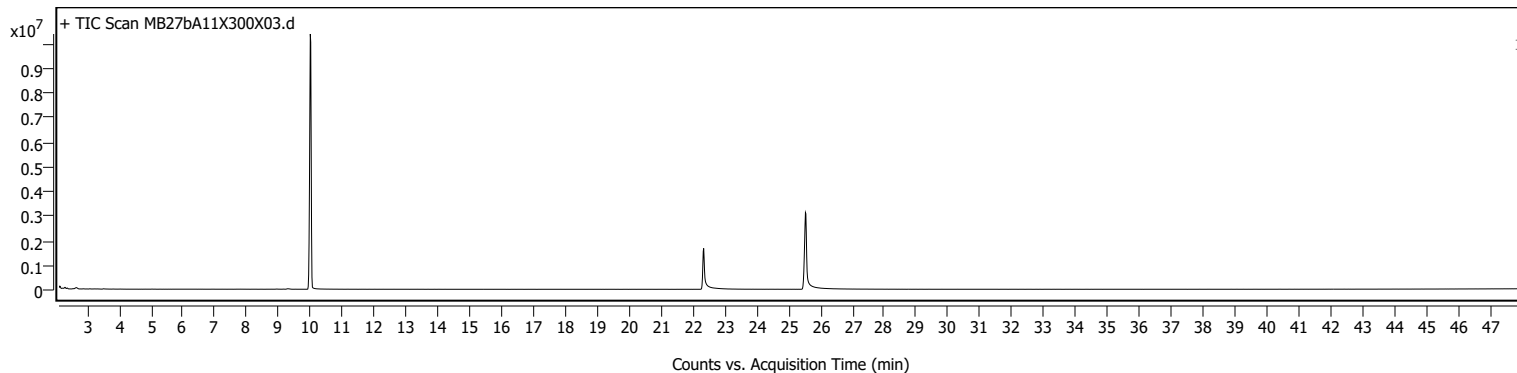

### Chromatogram Peaks

Peak	Start	RT	End	Height	Area	Area %	SNR
1	9.866	9.996	12.889	10348524	35170527	100.00	
2	22.088	22.336	25.085	1655411	8913269	25.34	
3	25.293	25.528	29.476	3108875	18593839	52.87	

MassHunter Qual 10.0  
(End of Report)