
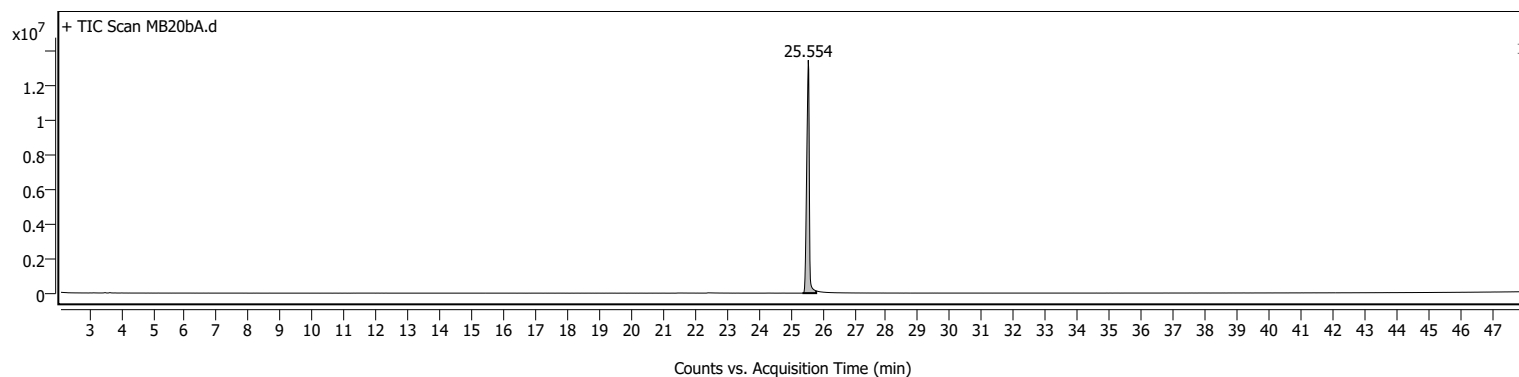


# Analysis Report

## Sample Information

Name	MB20bA	Data File Path	D:\MassHunter\GCMS\1\data\MB\MB20\MB20bA.D
Sample ID		Acq. Time (Local)	9/15/2022 7:36:09 PM (UTC+02:00)
Instrument	GCMS	Method Path (Acq)	D:\MassHunter\GCMS\1\methods\Standard HP 5 MS Temp 40 -320C_48min.M
MS Type	Q	Version (Acq SW)	MassHunter GC/MS Acquisition 10.0.384.1 14-Feb-2019 Copyright © 1989-2018 Agilent Technologies, Inc.
Inj. Vol. (ul)	0.5	IRM Status	
Position	131	Method Path (DA)	D:\MassHunter\GCMS\1\data\MB\MB20\MB20bA.D\Results\Qual\Version4\default.m
Plate Pos.		Target Source Path	
Operator		Result Summary	

## Sample Chromatograms

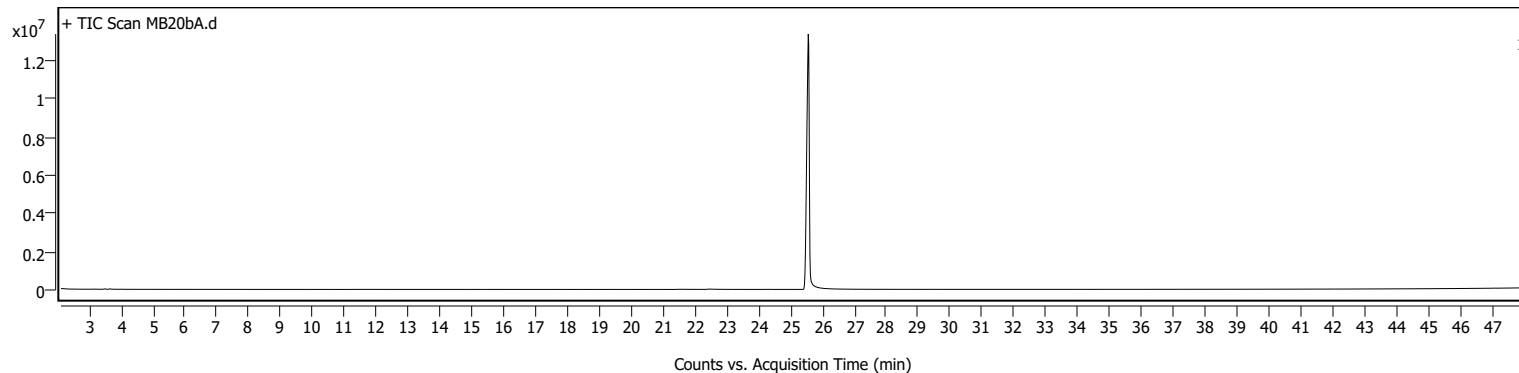


### Chromatogram Peaks

Peak	Start	RT	End	Height	Area	Area %	SNR
1	25.371	25.554	25.801	13368261	75767860	100.00	

## Sample Spectra

### + Scan (rt: 25.53 min)

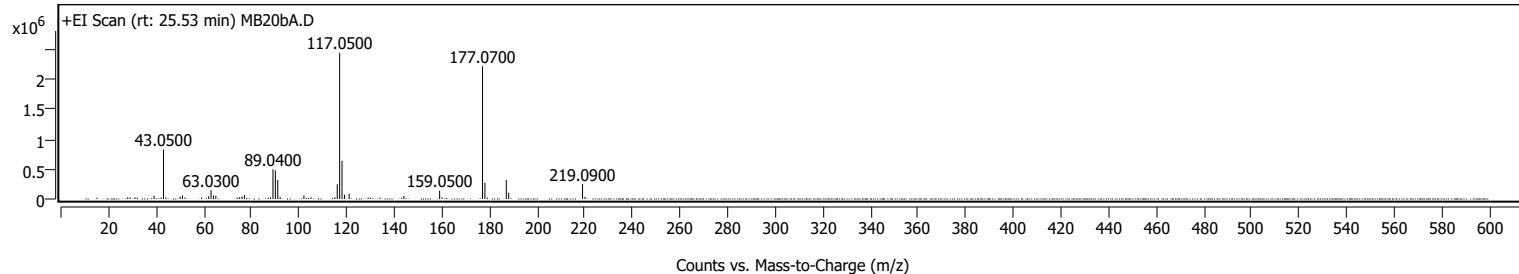

# Analysis Report



Agilent

Trusted Answers

## Spectrum Peaks

m/z	Z	Abund	Abund %	m/z (Calc)	Diff (ppm)	Ion Species	Formula	Ion Type
28.0500		29153	1.19					
31.0600		28540	1.17					
39.0600		54642	2.23					
43.0500	1	828179	33.85					
44.0400	1	24728	1.01					
50.0400		39297	1.61					
51.0400		59811	2.44					
62.0200		46533	1.90					
63.0300		146909	6.00					
64.0300		56961	2.33					
65.0400		54705	2.24					
74.0200		24922	1.02					
75.0300		30921	1.26					
76.0300		41648	1.70					
77.0400		66233	2.71					
88.0300		27725	1.13					
89.0400		495816	20.27					
90.0400		477967	19.54					
91.0500	1	317628	12.98					
92.0500	1	33310	1.36					
102.0400		60537	2.47					
105.0300		27866	1.14					
115.0400		29650	1.21					
116.0400		245809	10.05					
117.0500		2446609	100.00					
118.0500	1	639051	26.12					
119.0600	1	71519	2.92					
121.0500		88402	3.61					
129.0200		25582	1.05					
144.0300		49842	2.04					
159.0500	1	139308	5.69					
160.0500	1	27423	1.12					
177.0700	1	2218807	90.69					
178.0800	1	271059	11.08					
187.0500		320638	13.11					
188.0600		104287	4.26					
219.0900	1	250193	10.23					
220.1000	1	35138	1.44					

MassHunter Qual 10.0  
(End of Report)